



# 5 Biodiesel Samples Studied in 3 Labs by GC and 5 labs by Saftest

- 5 Biodiesel Samples Ranging from .07 to .22 were studied in 5 labs using the Saftest Testing System
- 5 Biodiesel, Samples were studied using GC in 3 Labs using the ASTM protocol
- Lab to Lab and Method to Method Results were compared.


# Mean Safetest Results vs Mean GC Results

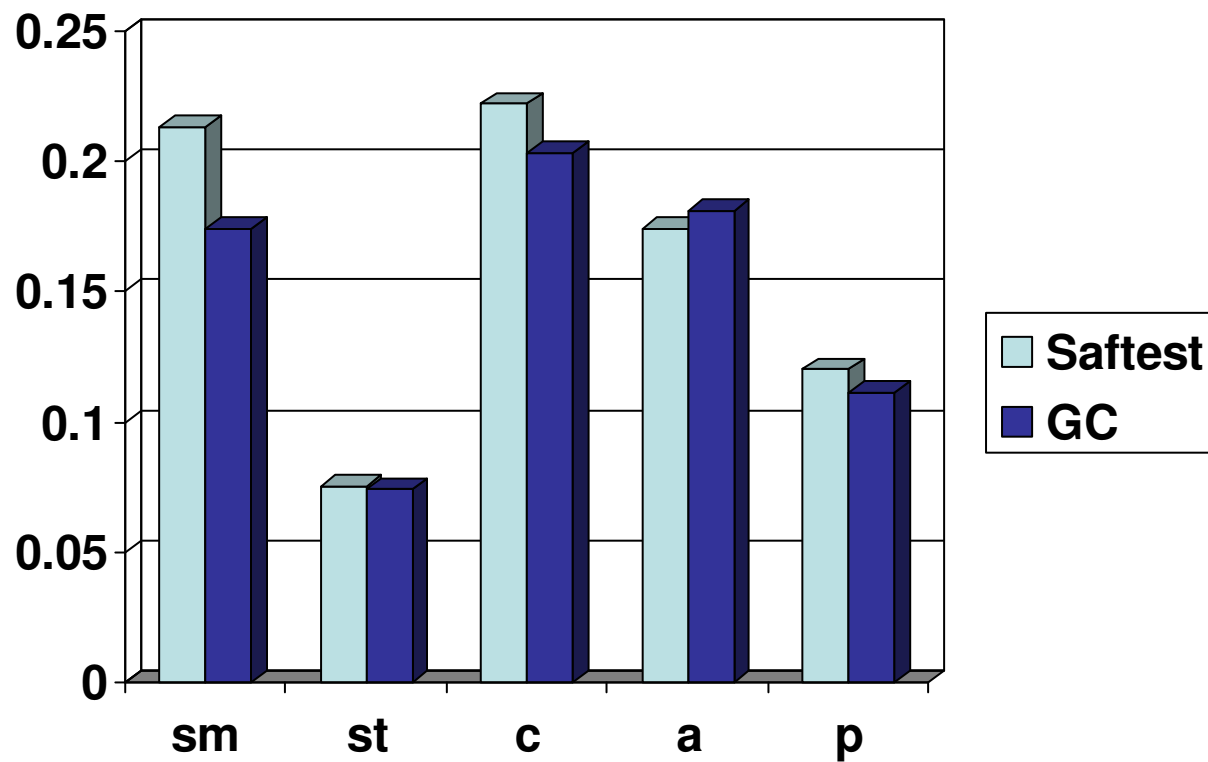

# (ASTM Total Glycerin vs Safatest Total Glycerin Round Robin 2007)

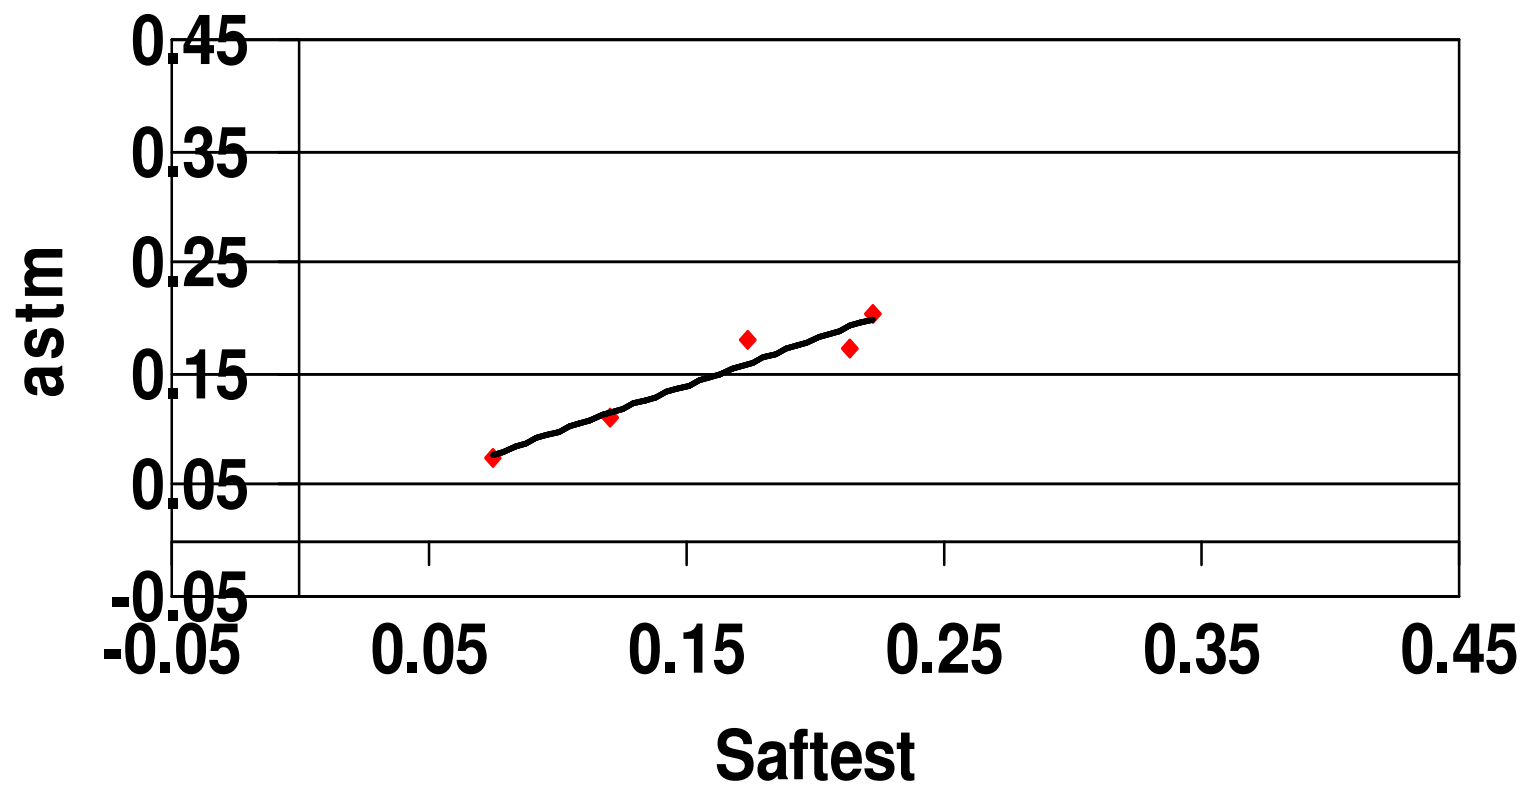

# Safest Results 5 Labs

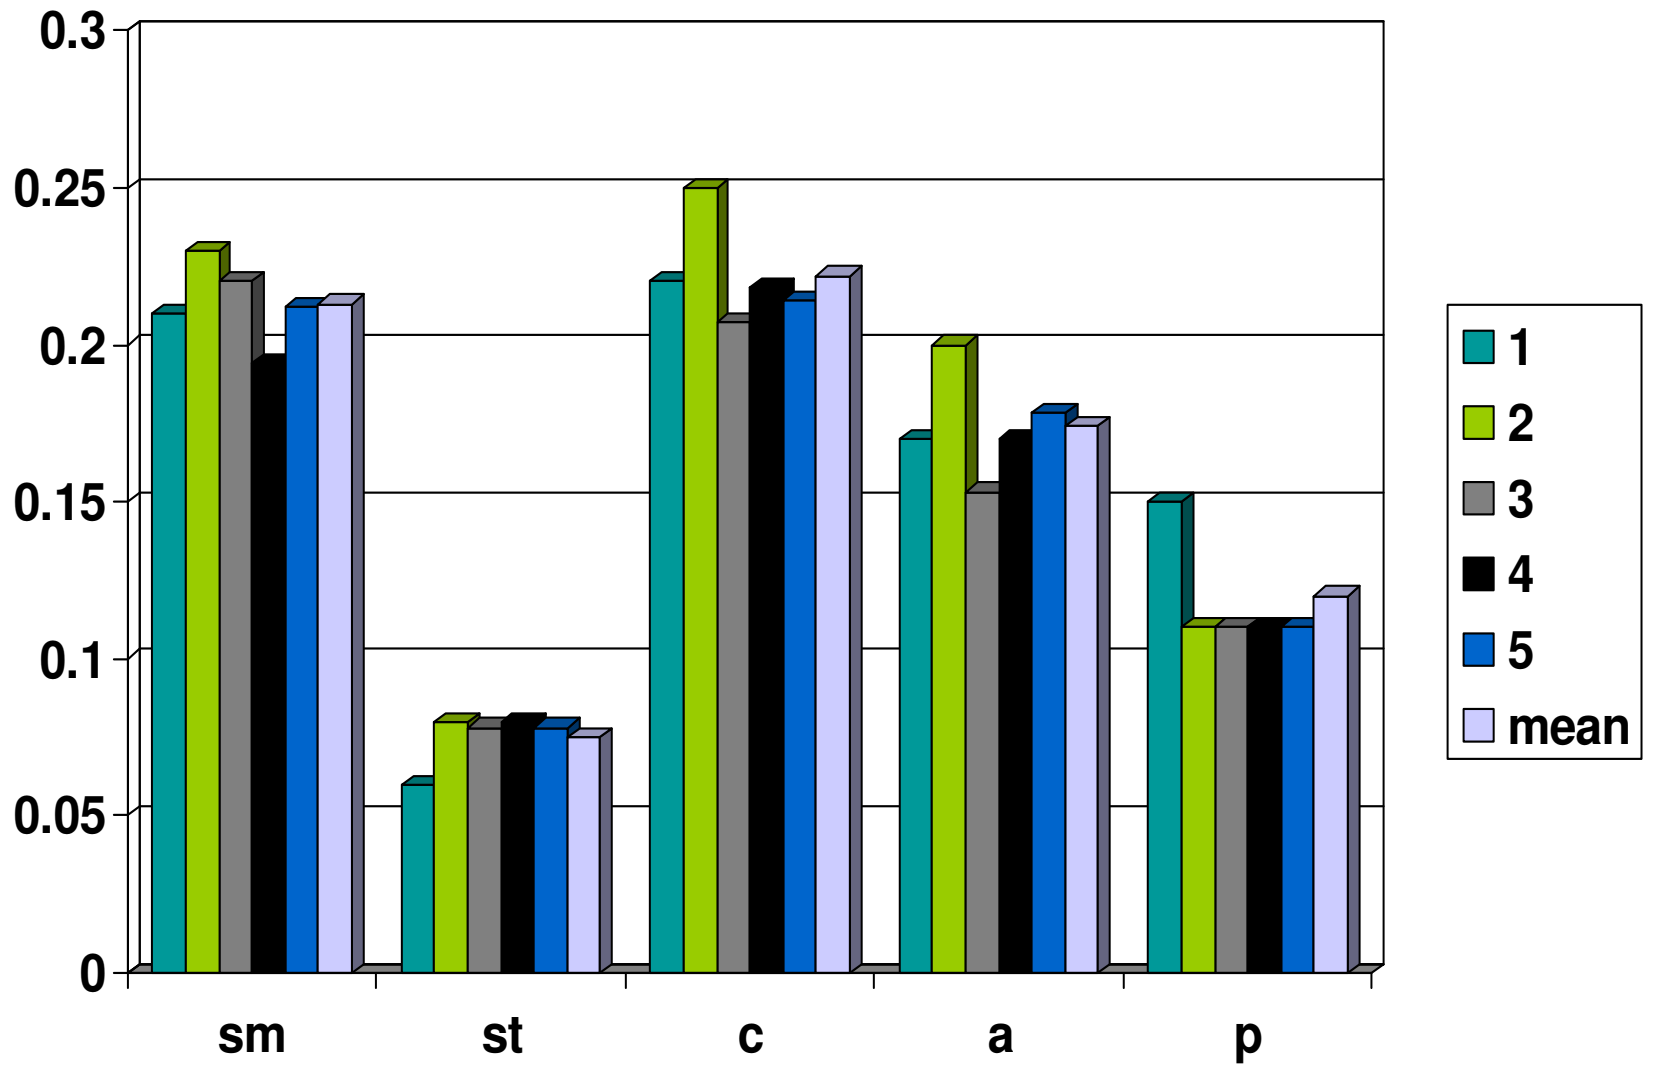

# GC Results 3 Labs

